

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
5 February 2004 (05.02.2004)


PCT

(10) International Publication Number  
**WO 2004/011084 A1**

- (51) International Patent Classification<sup>7</sup>: **A61N 1/18**,  
A61B 5/11, G01N 33/487
- (21) International Application Number:  
PCT/GB2003/003197
- (22) International Filing Date: 28 July 2003 (28.07.2003)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
0217554.5 30 July 2002 (30.07.2002) GB
- (71) Applicant (for all designated States except US): **AMERSHAM BIOSCIENCES UK LIMITED** [GB/GB];  
Amersham Place, Little Chalfont, Buckinghamshire HP7 9NA (GB).
- (72) Inventor; and  
(75) Inventor/Applicant (for US only): **CONLEY, Edward, Clarke** [GB/GB]; Amersham Biosciences UK Ltd, The Maynard Centre, Forest Farm Estate, Whitchurch, Cardiff, South Glamorgan CF14 7YT (GB).
- (74) Agents: **HAMMER, Catriona, MacLeod et al.**;  
Amersham plc, Amersham Place, Little Chalfont, Buckinghamshire HP7 9NA (GB).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),

[Continued on next page]

(54) Title: STIMULATING AND RECORDING DEVICE

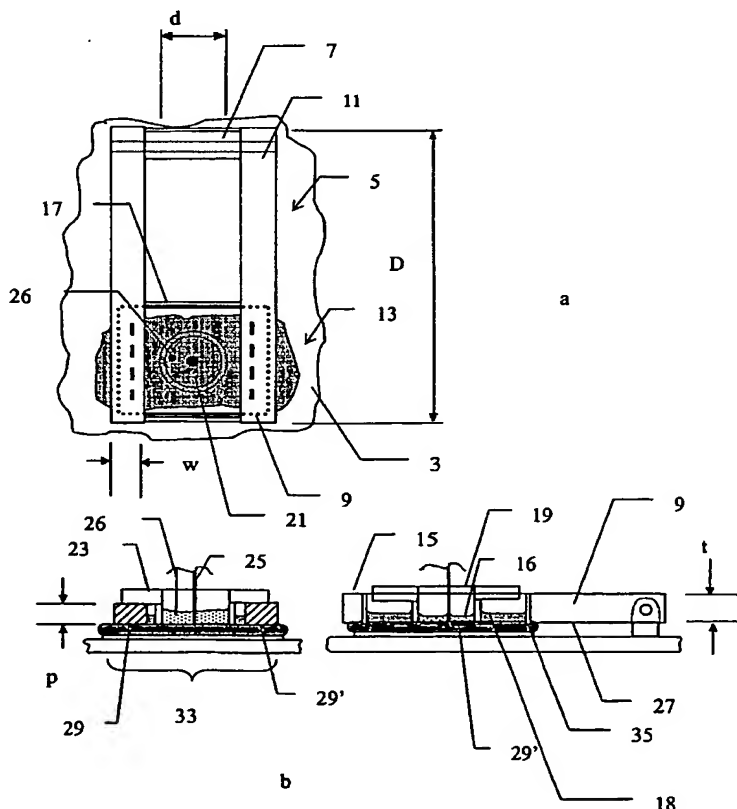

(57) **Abstract:** Device for stimulating a biological sample characterised in that it is provided with clamping means for clamping a sample, and electrodes for stimulating said sample, wherein said clamping means and electrodes are arranged such that when said biological sample is clamped by said clamping means, said electrodes substantially simultaneously penetrate said sample